OPERATING MANUAL

Chemical Resistant Diaphragm Pump

C300 / C400/ C410 / C510/ C600 / C610





WIGGENS GmbH

Gässlesweg 22-24, 75334 Straubenhardt, Germany

Tel.: 0049 7248 4529088

Wiggens Co., Ltd.

Room 426, Hall A, Office Building M8, No.1 Jiuxianqiao East Road, Chaoyang District, Beijing 100015, China

Tel: +86 400-809-2068

Fax: +86 400-809-2068-112

info@ wiggens.com www.wiggens.com

Congratulations!

You have made an excellent choice.

WIGGENS thanks you for the trust you have placed in us.

This operating manual has been designed to help you gain an understanding of the operation and possible applications of our instruments. For optimal utilization of all functions, we recommend that you thoroughly study this manual prior to beginning operation.

Unpacking and Inspecting

Please unpack the device carefully. Check that the package is right-side-up and then open it. Check that model of the product is one that you ordered. Check that there is no damage. If there is any damage, file a damage claim with the carrier. In the case of any damage a damage report should be requested immediately. These instructions must be followed fully for us to guarantee our full support of your claim for protecting against loss from concealed damage. The form required for filing such a claim will be provided by the carrier.

Changes without prior notification reserved

Important: keep operating manual for future use

Content

1.	Intended Use	4
2.	Operator Responsibility	4
	2.1. Disposal	5
	CE Conformity	5
	2.2. Technical Specifications	6
3.	Safety Instructions	7
	3.1. Explanation of Safety Notes	7
	3.2. For Your Protection	8
	3.3. For protection of the equipment	9
4.	Operating Procedures	10
	4.1. Environmental Operating Conditions	10
	4.3. Installation of the vacuum pump	11
	4.3.1. Operation Controls for C300	11
	4.3.2. Operation Controls for C400 and C600	12
	4.3.3. Operation Controls for C410 / C510 / C610	13
	4.4. Operation	13
	4.5. Parts List	14
	4.5.1. Parts of C300	14
	4.5.2. Parts of C400 / C600	15
	4.5.3. Parts of C410 / C510 / C610	16
5.	Cleaning and Maintenance	17
	5.1. Routine Cleaning	17
	5.2. Maintenance	18
6.	Transport and Storage	19
7.	Accessories and Spare Parts	19
	7.1. Chemical Resistant Vacuum Regulator / Filter Equipment	19
	7.2. Viton tubing	20
8.	Service	21
	8.1. Trouble-Shooting	21
	8.2. Warranty	21
	8.3. Contact/Technical Service	22

1. Intended Use

The C-Series Chemical Resistant Diaphragm Pumps are designed for laboratory use only.

All materials of the Chemical Resistant Diaphragm Pumps which have direct contact with gases are made of PTFE. They can be used in the chemical and petrochemical industry, the pharmacy industry and all industries that make use of chemical resistant vacuum processes, such as filtration, vacuum distillation, rotary evaporation, vacuum and centrifugal concentration, solid phase extraction, etc.

The Chemical Resistant Diaphragm Pumps' ultimate vacuum can reach a value as low as 2 mbar. They are working with noise less than 50 dB which is due to the special structure design.

All Chemical Resistant Diaphragm Pumps adopt an overheating protection system, which shuts down the pump when the inner temperature is too hot and automatically starts the pump again when cooled down to a safe temperature. This guarantees stable work of the pump and the safety of use. The Chemical Resistant Diaphragm Pumps can be integrated into vacuum filtration systems a diverse variety of accessories are available. The special design prevents solid impurities from accessing the pump head and thus guarantees the longevity of the pump.

2. Operator Responsibility

The products of WIGGENS ensure safe operation when installed, operated, and maintained according to common safety regulations. This section explains the potential dangers that may arise when operating the instrument and also specifies the most important safety precautions to preclude these dangers as far as possible.

- The operator is responsible for the qualification of the personnel operating the instrument.
- The personnel operating the instrument should be regularly instructed about the dangers involved with their job activities as well as measures to avert these dangers.
- Make sure all persons tasked with operating, installing, and maintaining the instrument have read and understand the safety information and operating instructions.
- When using hazardous materials or materials that could become hazardous, the instrument may be operated only by
 persons who are absolutely familiar with these materials and the instrument. These persons must be fully aware of
 possible risks.
- Only qualified personnel are authorized to perform configuration, installation, maintenance and repairs of the instrument.
- Routine operation can also be carried out by untrained personnel who should however be instructed by trained personnel.
- The safety of the user cannot be guaranteed if the appliance is operated with accessories that are not supplied or recommended by the manufacturer or if the appliance is operated improperly contrary to the manufacturer's specifications.

If you have any questions concerning the operation of your instrument or the information in this manual, please contact us!

2.1. Disposal



At the end of its service life the instrument is to be disposed of in accordance with the local regulations specified for the disposal of electronic industry waste in an environmentally friendly manner.

CE Conformity

	The products described in the operating instructions conform to the requirements of the following	
European guidelines:		
	Low voltage regulations with respect to legal harmonization of the member countries concerning	
	electric devices for use within certain voltage limits.	
	EMC guideline with respect to legal harmonization of the member countries concerning	
	electromagnetic compatibility.	
APPROVALS	EN61326-1: 2013, 014/30/EU	
European	EN61010-1:2010, 2014/35/EU	
	EN60204-1: 2006, 2006/42/EC	
	EN50581: 2012, 2011/65/EU	

2.2. Technical Specifications

Model	C300	C400	C410
Maximum Flow Rate (L/min)	22	34	25
Ultimate Vacuum(mbar)	100	120	13
Outlet (mm)	10	10	10
Maximum Continuous Pressure		1 Bar (14.7 psi)	
Power (W)	70/60	90/95	90/95
Mains(Voltage/Frequency)	/oltage/Frequency) 115V,60Hz/ 220V, 50Hz		
Permissible Ambient Temperature +5+40°C			
Permissible Temperature of Pumped Gas +5+40°C			
Weight (kg)	6	8.5	8.5
Basic Order Number	169300	169400	169410

Model	C510	C600	C610
Maximum Flow Rate (L/min)	41/34	60	34
Ultimate Vacuum(mbar)	8	90	2-4
Outlet (mm)	10	10	10
Maximum Continuous Pressure		1 Bar (14.7 psi)	
Power (W)	250/245	250/270	250/245
Mains(Voltage/Frequency)	220V, !	50Hz or 220V, 60Hz or110	OV,60Hz
Permissible Ambient Temperature		+5+40°C	
Permissible Temperature of Pumped Gas		+5+40°C	
Weight (kg)	13.2	13.2	13.8
Basic Order Number	169510	169600	169610

All measurements have been carried out at the stated voltage, frequency, and an ambient temperature of 25°C. Technical changes without prior notification reserved.



WIGGENS Order Numbers consist of the Basic Order Number (BON) and the Order Number Addition (ONA) which explains different characteristics of the product that can vary from country to country. Order Numbers as stated on the product label and box label are stated as Full Order Numbers (FON), consisting of the BON followed by the ONA. For a full explanation of the ONA of your product, please ask your local WIGGENS support or refer to the Order Number Guide in the *WIGGENS* General Catalog.

3. Safety Instructions

3.1. Explanation of Safety Notes

In addition to the safety warnings listed, warnings are posted throughout the operating manual. These warnings are designated by an exclamation mark inside an equilateral triangle. "Warning of a dangerous situation (Attention! Please follow the documentation)."

Symbol	Additional term / Description
Warning signs	The danger is classified using a signal word. Read and follow these important instructions for
A	averting dangers.
	Warning!
	Describes a possibly highly dangerous situation. If these instructions are not followed, serious
	injury and danger to life could result.
	Caution!
	Describes a possibly dangerous situation. If this is not avoided, slight or minor injuries could
	result. A warning of possible property damage may also be contained in the text.
	Notice!
	Describes a possibly harmful situation. If this is not avoided, the product or anything in its
	surroundings can be damaged.
	Note!
(S)	Draws attention to something special.
	Important!
$lue{\mathbf{U}}$	Indicates usage tips and other useful information.

3.2. For Your Protection

- Make sure you read and understand all instructions and safety precautions listed in this manual before installing or operating your instrument.
- Keep the operation instructions in a place where they can be accessed by everyone.
- Connect the instrument to a power socket with earthing contact (PE-protective earth)!
- The power supply plug serves as a safe disconnecting device from the line and must always be easily accessible.
- Do not stay in the area below the instrument.
- Make sure the product is checked for proper condition regularly (depending on the conditions of use). Regularly
 check (at least every 2 months) the proper condition of the mandatory, warning, prohibition and safety labels.
- Never operate damaged equipment.
- Always turn off the instrument and disconnect the mains cable from the power source before performing any service
 or maintenance procedures, or before moving the instrument.
- Transport the instrument with care.
- Never operate instruments with damaged mains power cables.
- Observe all warning labels.
- Never remove warning labels.
- Repairs are to be carried out only by qualified service personnel
- Warning! Never use the pump with any flammable gas or toxic material.
- Warning! Before using a medium, check the compatibility of the materials of the pump head, diaphragm and valves with the medium.
- Warning! Before using a medium, check whether the medium can be transferred anger-free in the specific application case.
- Warning! Ensure that the system is not subject to any risks of explosion, also in extreme operating situations (temperature, pressure) or in case of malfunctions.
- Warning! Only transfer gases which remain stable under the pressures and temperatures occurring in the pump.
- Laboratory equipment or additional components connected to a pump have to be suitable for use with the pneumatic capabilities of the pump
- Warning! Make sure the temperature of the medium is always sufficiently below the ignition temperature of the medium, to avoid ignition or explosion.
- If necessary, consider any external sources of energy, such as radiation, that may add heat to the medium.

3.3. For protection of the equipment

- You have received a product designed for industrial and experimental use. Nevertheless, avoid strikes to the housing, vibrations, damage to the operating-element panel, and contamination.
- Make sure that the mains power supply has low impedance to avoid any negative effects on instruments being operated on the same mains.
- Do not expose the unit to sunlight.
- Sudden drops may cause damage in the interior of the instrument.
- When finished with the pumping operation, do not turn off the pump at once but continue to run the vacuum pump
 for at least two minutes in order to draw out the mist and tiny liquids to prolong the service life of the pump.
- The filter cartridge (optional) is used to absorb moisture and dust. Replace it when it is saturated to maintain a high pumping efficiency.
- Never use the pump with any flammable gas or toxic material.
- Press the power switch to interrupt the pump, rather than disconnect the main power plug directly.
- When in an emergency, disconnect the main power plug.
- Protect the pump from vibrations, jolts and external damage.
- The pump is not suitable for use underground.
- The pump is not suitable for transferring dusts.
- The pump is not suitable for transferring liquids.
- Warning! An overpressure must not be applied to the suction side of the pump.
- The pumps must not be modified. If a wearing part is replaced, the original function of the pump must be checked by reaching the specified ultimate vacuum

4. Operating Procedures


4.1. Environmental Operating Conditions

The pump must operate in the following conditions:

- Indoors
- Altitudes up to 2000 meters
- Temperatures from +5°C to +40°C
- Maximum relative humidity 80% for temperatures up to +31°C, linear decrease down to 50% relative humidity at a temperature of +40°C
- Max. mains fluctuation of ± 10 % are permissible
- Overvoltage category II

4.2. Design and Function





Index	Description	
1	Outlet valve	
2	Inlet valve	
3	Transfer chamber	
4	Diaphragm	
5	Eccentric	
6	Connecting rod	
7	Pump drive	


Diaphragm pumps transfer, compress (depending on pump version) and evacuate gases and vapors.

The elastic diaphragm (4) is moved up and down by the eccentric (5) and the connecting rod (6). In the downward stroke it aspirates the gas to be transferred via the inlet valve (2). In the upward stroke, the diaphragm presses the medium out of the pump head via the outlet valve (1). The transfer chamber (3) is hermetically separated from the pump drive (7) by the diaphragm.

4.3. Installation of the vacuum pump


- 1. Place the vacuum pump on a stable, flat surface and proper environment for operation.
- 2. Check the voltage specified on the rear label at the bottom of the unit. Make sure that it matches the mains requirements in your country.
- 3. To enable the suction function, connect the inlet of the pump to the outlet of your objective equipment with high-pressure tubing.

4.3.1. Operation Controls for C300

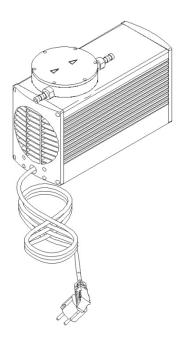


- 1. The diagram of the pump system is shown above.
- 2. When all tubes have been properly connected to the Inlet and Outlet, activate the pumping function by pressing the On/Off Button.
- 3. For vacuum monitoring and regulation, an optional vacuum regulator / moisture trap is needed.

4.3.2. Operation Controls for C400 and C600

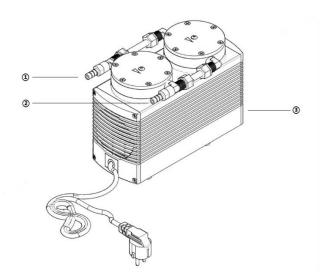

- 1. The diagram of the pump system is shown above.
- 2. When all tubes have been properly connected to the Inlet (1) and Outlet (2), activate the pumping function by pressing the on/Off Button (3).
- 3. For vacuum monitoring and regulation, an optional vacuum regulator / moisture trap is needed.

4.3.3. Operation Controls for C410 / C510 / C610



- 1. The diagram of the pump system is shown above.
- 2. When all tubes have been properly connected to the Inlet (1) and Outlet (2), activate the pumping function by pressing the On/Off Button (3).
- 3. For vacuum monitoring and regulation, an optional vacuum regulator / moisture trap is needed.

4.4. Operation




Warning:

When the pump is used in water filtration, prevent the liquid level in the flask / waste bottle from exceeding the safety level. Failure to comply can result in serious damage to the pump and void the warranty.


4.5. Parts List

4.5.1. Parts of C300

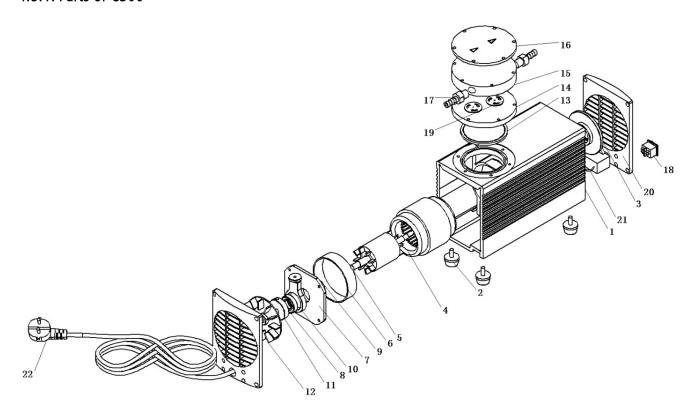


Index	Description	Quantity	Index	Description	Quantity
1	Body	1	12	Cooling Fan	1
2	Rubber Stand	4	13	Diaphragm	1
3	Cover	1	14	Diaphragm Block	1
4	Motor	1	15	Diaphragm Head	1
5	Motor	1	16	Aluminum plate	1
6	Locating ring	1	17	Tier Connector	2
7	Cover	1	18	On/Off Switch	1
8	Bearing	1	19	Valve Plate	2
9	Bearing	2	20	Front Body Lid	2
10	Connecting Rod	1	21	Condenser	1
11	Counterweight	1	22	Plug	1

4.5.2. Parts of C400 / C600

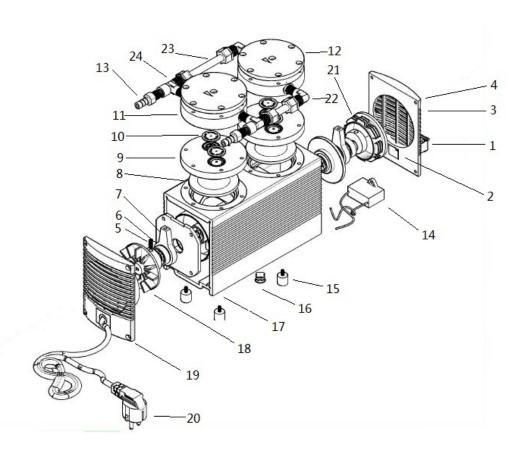

Index	Description	Quantity	Index	Description	Quantity
1	On/Off Switch Cup	1	13	Tier Connector	2
2	On/Off Switch	1	14	Condenser	1
3	Front Body Lid	1	15	Rubber Stand	4
4	Set Screw	8	16	Clog	1
5	Counterweight	2	17	Body	1
6	Bearing	2	18	Cooling Fan	1
7	Connecting Rod	2	19	Rear Body Lid	1
8	Diaphragm	2	20	Plug	1
9	Diaphragm Block	2	21	Piston Set Cover	1
10	DiaphragmValve	4	22	L-Connector	2
11	Diaphragm Head	2	23	Interflow Tube	2
12	Stainless Plate	2	24	T-Connector	2

4.5.3. Parts of C410 / C510 / C610

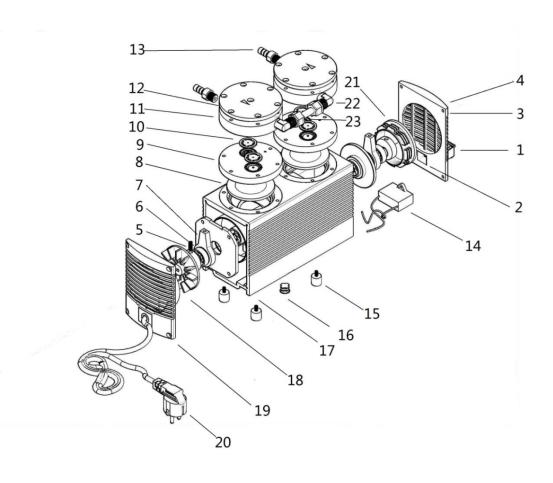


Index	Description	Quantity	Index	Description	Quantity
1	On/Off Switch Cup	1	13	Tier Connector	2
2	On/Off Switch	1	14	Condenser	1
3	Front Body Lid	1	15	Rubber Stand	4
4	Set Screw	8	16	Clog	1
5	Counterweight	2	17	Body	1
6	Bearing	2	18	Cooling Fan	1
7	Connecting Rod	2	19	Rear Body Lid	1
8	Diaphragm	2	20	Plug	1
9	Diaphragm Block	2	21	Piston set Cover	1
10	Diaphragm Valve	4	22	L-Connector	2
11	Diaphragm Head	2	23	Interflow Tube	1
12	Stainless Plate	2			

5. Cleaning and Maintenance

5.1. Routine Cleaning

The device is maintenance-free.

Cleaning



For cleaning disconnect the main plug.

Before switching off the pump, flush it with air (if necessary for safety reasons: with an inert gas) for about five minutes under atmospheric conditions (ambient pressure).

Only use solvents for cleaning if the head materials cannot be attacked (check the resistance of the material!).

If compressed air is available, blow out the components.

Only use cleansing agents which have been recommended by WIGGENS

Use to remove:

Dyesisopropyl alcohol

Construction materials isopropyl alcohol/water containing surfactant
Cosmetics isopropyl alcohol/water containing surfactant

Foodstuffs water containing surfactant

Fuels water containing surfactant

- Do not allow moisture to get into the appliance when cleaning.
- Wear protective gloves when cleaning the devices.
- -Before using another than the recommended method for cleaning or decontamination,

the user must ascertain with WIGGENS that this method does not destroy the instrument



Note:

- Do not use chlorine bleach, chlorine-based cleanser, abrasives, ammonia, steel wool or scouring pads with metal content or similar harsh solvents or abrasives. These may damage the surface of the instrument.
- When cleaning, make sure that no liquids enter the inside of the housing.

5.2. Maintenance

Do not attempt to service or repair a WIGGENS overhead stirrer. If the overhead stirrer housing is opened the warranty becomes void. Contact WIGGENS for return authorization and return instructions.

Ordering spare parts

When ordering spare parts, please give:

- Machine type
- Manufacturing number, see type plate
- Item number and designation of the spare part.

Repair

Please only send devices in for repair that have been cleaned and are free of materials which might present health hazards. For this, use the "certificate of compliance" form which you can obtain from WIGGENS. If your appliance requires repair, return it in its original packaging. Storage packaging is not sufficient when sending the device - also use appropriate transport packaging.

6. Transport and Storage

- Clean the pump so that it is free from any materials which may be harmful to the health. Provide a material safety data sheet where appropriate.
- Place the pump unit and its parts into the original packing or a container with necessary protection to prevent damage during transport. Seal the original packing or container with packing tape.
- Store the packed unit in a dry place.



CAUTION!

Failure to clean, maintenance, and handle the pump as outlined can lead to damages or be harmful to the health.

7. Accessories and Spare Parts

7.1. Chemical Resistant Vacuum Regulator / Filter Equipment

Model	Description	Order No.
	Set 1 (includes vacuum trap and regulator)	169311-06
SE	Set 2 (includes vacuum trap only)	169312-06
Chemical Resistant Vacuum Regulator	Set 3 (neither include vacuum trap nor regulator)	169313-06

7.2. Viton tubing

Model	description	Order No.
	Outer Diamete: 12 mm	
	Inner Diameter:6mm	168000-01
	Thickness:3mm	100000-01
	Length:1m	
	Outer Diamete: 14mm	
	Inner Diameter:8mm	168001-01
	Thickness:3mm	100001-01
	Length:1m	
	Outer Diamete: 16mm	
Viton tubing	Inner Diameter:10mm	160002 01
	Thickness:3mm	168002-01
	Length:1m	



Note: Length upon request (min. 1 m)



Note! For more information about Accessories please contact your local supplier



CAUTION!

For safety and guarantee reasons only original accessory parts are to be used!

8. Service

8.1. Trouble-Shooting

Cause	Remedy		
The pump does not react after turning on the On / Off Switch	 Ensure that the mains electricity plug is plugged into a working socket outlet and check if the On / Off Switch is in the "on" position. If the On / Off Switch is in the "on" position, release the vacuum, disconnect the pump from the power source and let the pump cool down, and investigate the reason for overheating 		
	3. After cooling down, connect the pump to the power source and try again4. If there is no reaction after several attempts, please contact the WIGGENS support.		
The pump does not reach the designated ultimate vacuum	 Check if all tubing is tight and if there is a leakage at any point Disconnect the pump from all other sources, connect it directly to a vacuum controller / vacuum gauge, and block the gas intake If the pump still does not reach the designated ultimate vacuum, please contact the WIGGENS support. Diaphragms, valve plates, or seal rings might be worn out. 		



WIGGENS reserves the right to carry out technical modifications with repairs for providing improved performance of the instrument.

8.2. Warranty

In accordance with *WIGGENS* warranty conditions, the warranty period is 24 months. For claims under the warranty please contact your local dealer. You may also send the machine direct to our works, enclosing the delivery invoice and giving reasons for the claim. You will be liable for freight costs. The warranty does not cover wearing parts, nor does it apply to faults resulting from improper use or insufficient care and maintenance contrary to the instructions in this operating manual.

WIGGENS reserves the right to decide the validity of any warranty claim. In case of faults arising either due to faulty materials or workmanship, parts will be repaired or replaced free of charge.

Any other compensation claims, such as consumables, damages caused by corrosion or accidental breakage, are excluded from this guarantee.

This warranty may only be altered by a specifically published amendment. No individual has authorization to alter the provisions of this warranty policy or its amendments.

8.3. Contact/Technical Service

If your device is not working properly:

Please inform *WIGGENS* Instruments by using our contact information.

You have contacted *WIGGENS* Instruments?

- Copy and complete the Conformation of condition of unit from these operating instructions.
- Please repack the device appropriately for transport and send to *WIGGENS* Instruments together with the Confirmation of condition of unit.

Our contact details

WIGGENS GmbH

Add: Gässlesweg 22-24, 75334 Straubenhardt, Germany

Tel.: 0049 7248 4529088

Wiggens Co., Ltd.

Room 426, Hall A, Office Building M8, No.1 Jiuxianqiao East Road, Chaoyang District, Beijing 100015, China

Tel: +86 400-809-2068

Fax: +86 400-809-2068-112

info@ wiggens.com

service@wiggens.com

www.wiggens.com

Confirmation of condition of unit

In the case of repair, copy and complete the Conformation of condition of unit and send it to WIGGENS Instruments. 1. Details about the unit Product number Serial number Reason for repair 2. Has the device been cleaned, decontaminated/sterilized? Yes No 3. Is the unit in a condition which does not represent any health threats for the staff of our service department? Yes No If not, which substances has the unit come into contact with? 4. Legally binding declaration The customer is aware of being legally liable to WIGGENS Instruments for any damages arising from incomplete and incorrect information. Date Signature Company stamp Please Note The shipper is responsible for the return of the goods in well-packed condition, suitable for the mode of transport. Sender information Name, first name Company Department, research group Street Zip code, city Country

Phone E-mail



WIGGENS GmbH

Gässlesweg 22-24, 75334 Straubenhardt, Germany

Tel.: 0049 7248 4529088

WIGGENS China

Room 426, Hall A, Office Building M8, No.1 Jiuxianqiao East Road,

Chaoyang District, Beijing 100015, China

Tel: +86 400-809-2068

Fax: +86 400-809-2068-112

info@ wiggens.com

www.wiggens.com